


Oscilla[®] SM930 Screening Memory audiometer

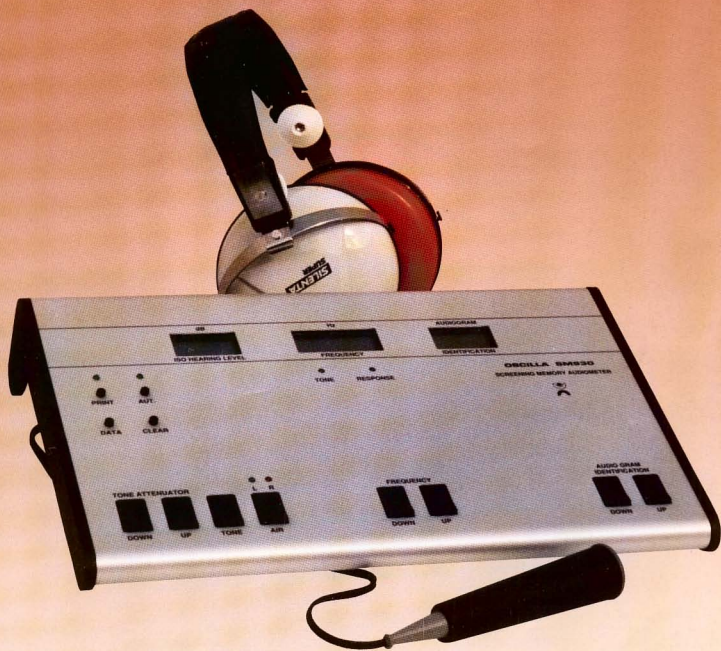

Includes:

Hughson Westlake

SPECIAL FEATURES

Oscilla® SM930 Screening Memory audiometer equipped with a host of features making it extremely advanced and at the same time focusing on ease - of - use. **Oscilla® SM930 Screening Memory audiometer** contains storage capacity of 90 audiograms, which all may be stored for later printout or transfer to patient file. The programmed values are stored in the internal memory, and naturally kept even if the unit is turned off.

Together with your **Oscilla® SM930 Screening Memory audiometer** you may have a special designed software program: audioVGAwin designed by Inmedico; which cheap and very easy makes it possible for the users to create their own patient file system. In addition the **Oscilla® SM930 Screening Memory audiometer** transfer test results in a format, which makes it possible to transfer data to patient file systems already existing.

By printing or transfer to PC the device automatically selects the correct symbols for left or right ear, and in addition you may choose manual or automatic transfer/printing.

Do you want a printout you may perform it just after finished test OR you may wait until later, when it is convenient - the audiometer has stored all values.

You may follow the results on the screen during the test in two ways: each time you press the DATA button, or AUTOMATICALLY by using one of the set-up functions.

All functions are controlled by an advanced microprocessor, which offers stability and durability. The built-in tone generator is crystal driven avoiding distortion and making it insensitive to temperature fluctuations.

The **Oscilla® SM930 Screening Memory audiometer** may perform either manual or fully automatic hearing test, having four automatic tests allowing individually designed threshold test.

Technical specifications:

Frequencies : 11 fixed frequencies from 125 Hz to 8000 Hz.
Hearing Level Range : - 10 dB to 110 dB in 5 dB steps.

Maximum intensities:

Frequency Hz	125	250	500	750	1000	1500	2000	3000	4000	6000	8000
Air conduction dB	70	90	110	110	110	110	110	110	110	100	90

Program : Manual or automatic test.
Printer interface : Automatic printout.
Serial interface : Automatic transfer - 9600 baud.
Calibration : Digital calibration in accordance with international standard (EN60645-1).
Power Supply : Mains adapter for 220-240 V AC.
Dimensions : 295mm x 180mm x 55mm.
Weight : Approx. 1 kg.
Standard accessories : Noise excluding headsets fitted with TDH-39 earphones, patient signal & adapter.
Optional extras : Carrying bag. Parallel and/or serial cable. Software.

Setup:

In this position you may change some of the pre-set functions. The program will save the last entry until a new change is made. The setup function has the following possibilities:

- Mode 1) Each of the 11 frequencies can be connected or disconnected.
- Mode 2) Automatic length of tone of 0, 0.5, 1.0 or 1.5 seconds.
- Mode 3) Connecting/disconnecting storage function, and you may choose manual or automatic data transfer.
- Mode 4) Choice between variable, 20 dB, random automatic threshold test or Hughson Westlake. Alarm after finished test.
- Mode 5) Selection of printer: 9 or 24 pin, Epson compatibles, IBM, Laser, HP printers or IBM Pro printer.
- Mode 6) The option of a special IBM printer.
- Mode 7) Right & Left printed on the same audiogram or on two separate audiograms.
- Mode 8) Automatic print-out after finished test.
- Mode 9) Option of setting top-margin on the printout.
- Mode 10) Back to basic value in Hughson Westlake by change of frequency (together with mode 13).
- Mode 11) Hughson Westlake minimum (-10dB to 40 dB).
- Mode 12) Hughson Westlake maximum (50 dB to 80 dB).
- Mode 13) Hughson Westlake basic level (0dB to 50 dB).
- Mode 14) Connection/disconnection of the key to AudioConsole.

Distributed: Paxton Barrand Electromedics
283 George Street, Sydney N.S.W. 2000 - Australia
www.paxtonbarrand.com.au

Manufactured: Inmedico
8520 Lystrup - Denmark
www.inmedico.com